


Broomfield		
VascLab		
Hosp Number	Consultant YOW	Date exam 28-05-2019

LOWER LIMB COLOUR DUPLEX VENOUS ASSESSMENT

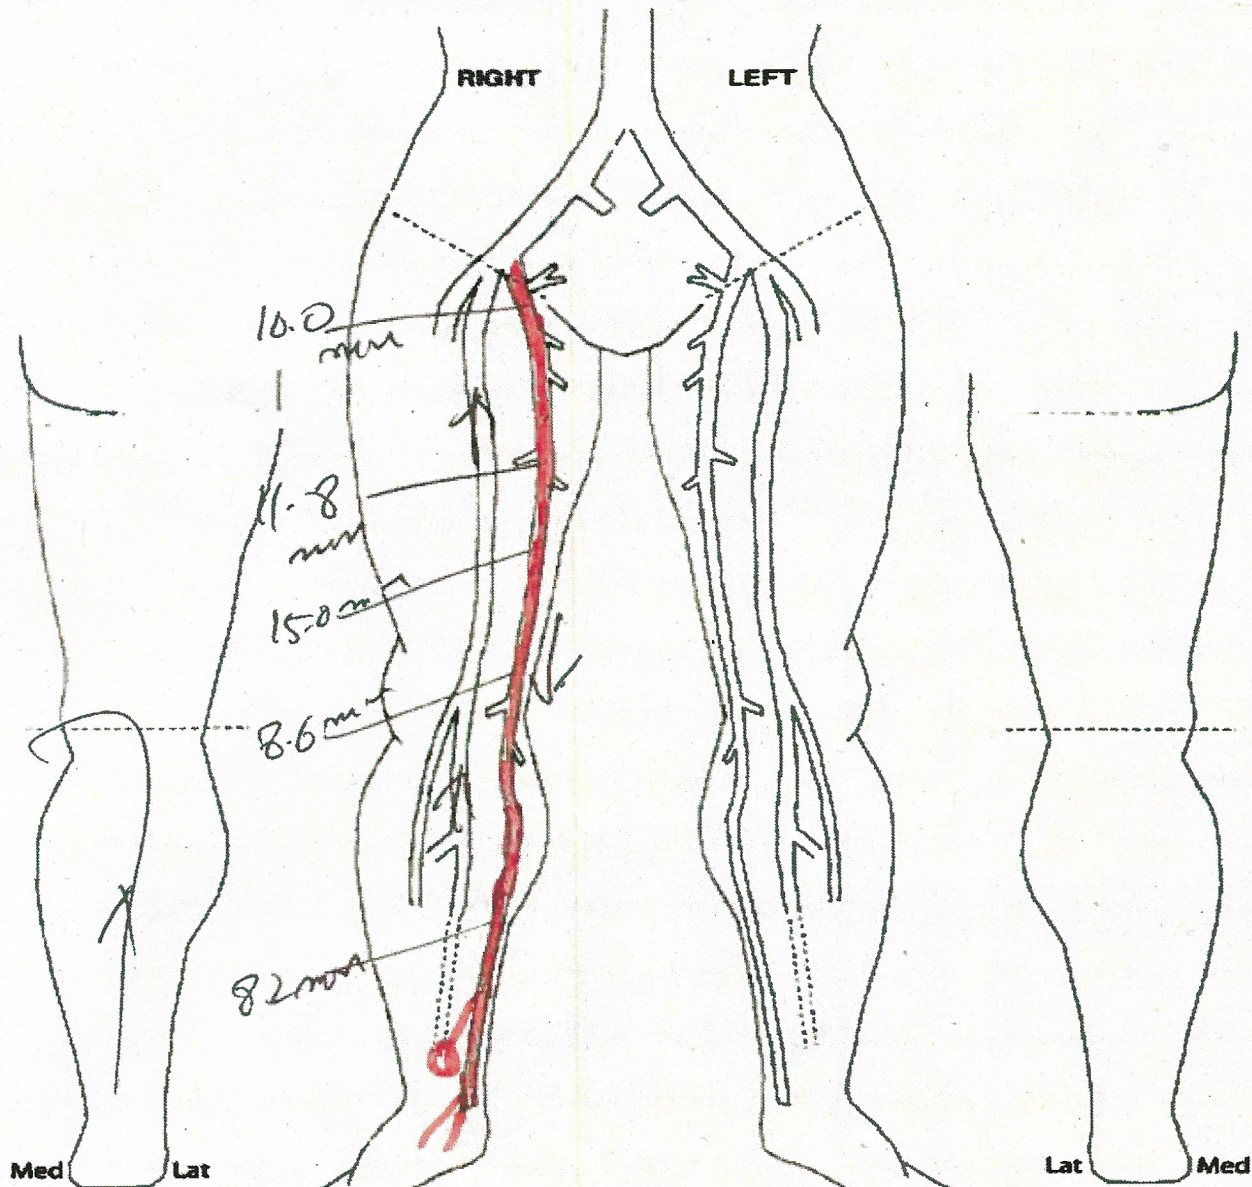

Right;

LSV is incompetent from SFJ in its entirety, diameter is 8.2mm to 15mm. it is rather straight. It also drain in a perforator 8cm above medial malleolus.

SSV and deep veins are patent and competent.

Scan performed and reported by: Ikhlaiq Rana